
20 YEARS DSADetection
SINGLE FOCUS. SINGLE SOURCE.

TRACE DETECTION CONSUMABLES

Product Catalog

2026

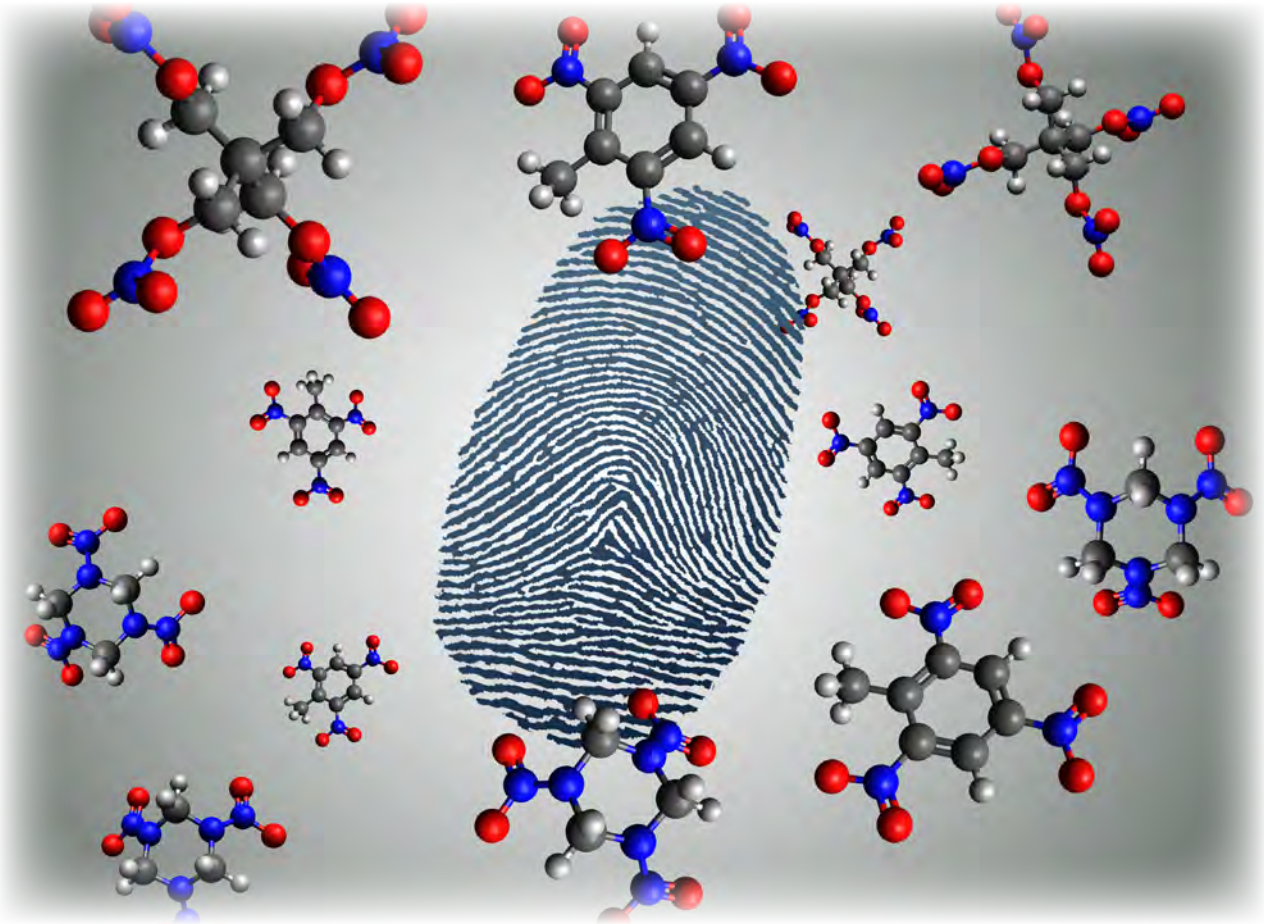


Sandia National Laboratories

Airports UK

ACI EUROPE

Table of Contents

6 Cotton Swabs (100ct)
6 Bumper Feet
6 Fan Filter Replacement, 5pk
7 Sieve Canister X-Ring (#019)
7 Sieve Canister X-Ring (#012)
7 Thermal Paper Roll, 112 mm
8 Verification Sample A - Negative
8 Verification Sample, B - Positive
8 Filter Screen, Sample Pathway
9 Filter Screen, Sample Pathway (5ct)
9 Orifice Filter Replacement Tool
9 Sieve Canister (4-pack) with Filter
10 Sieve Canister (12-pack) with Filters
10 Alcohol Wipes, 1.7x3.5 (100ct)
10 Calibration Traps, Dual (25ct)
11 B220 Checkpoint Sample Traps (100ct)
11 B220 Checkpoint Sample Traps (300ct)
11 Cargo Sample Traps (100ct)
12 Cargo Sample Traps (300ct)
12 Dual Mode Verification Trap (25ct)
12 Dual Mode Verification Trap (100ct)
13 QS-H150E Sieve Canister
13 Thermal Printer Paper (80mm)
13 Thermal Printer Paper (pkg of 5)
14 Printer Paper
14 Printer Ribbon
14 500DT Hand Swab (100ct)
15 500DT Hand Swabs (200ct)
15 500DT Sample Swabs (200ct)
15 500DT Sample Swabs (400ct)
16 Sampling Wand Velcro Hook (10ct)
16 Verification Pen
16 Clearing Dropper
17 Sampling Wand Velcro Shaper (10ct)
17 Itemiser® DX Starter Consumable Kit
17 Calibration Pen
18 Clearing Spray
18 Calibration Traps (25ct)
18 Calibration Traps (100ct)
19 N-Mode Dopant, Long Life Positive Ion
19 N-Mode Dopant, Long Life Positive Ion
19 Sample Filter and Purge Inlet Filter
20 Fan Filter
20 Fan Guard
20 Fan Filter Kit
21 Fuse, 250V AC 3.15A
21 Fuse, 15A, 32V 3AG, for DC input
21 Nozzle Screen Kit
22 O-Ring Silicone (#019)
22 O-Ring Viton (#008)
22 Thermal Printer Paper
23 Spare Parts Kit
23 Itemiser® 3/DX Spare Parts Kit
23 Sample Traps (25ct)
24 Itemiser Sample Traps (100ct)
24 Itemiser Sample Traps (300ct)
24 Verification Pen
25 Verification Traps (100ct)
25 Verification Traps (25ct)
25 Check Sample Vial - Military
26 Sintered Filter
26 Condenser Tube
26 Foam Filter
27 Behind Bottle Foam Filter
27 Fan Guard, 4-Prong
27 Behind Bottle Cover and Filter
28 Filter Kit
28 O-ring, Viton (#009)
28 O-ring, Viton (#012)
29 400B Printer Paper, Intl
29 Swab Sampler Velcro Hook (10ct)
29 CW/TIC Vapor Verific
30 Verification Pen
30 Membrane Kit
30 O-Ring Silicone (#022)
31 Canned Air
31 Standard Bin Cart
31 Safety Enclosure Cleaning Cloth
32 ETD Mobile Workstation (powered)
32 ETD Mobile Powered Workstation LiFePO4
32 Replacement Batteries for Mobile Workstation (2pk)
33 Inverter/Charger 1000w, Mobile Workstation
33 LiFePO4 Battery
33 Small, Powder-Free, Nitrile Gloves (4mil)
34 Medium, Powder-Free, Nitrile Gloves (4mil)
34 Large, Powder-Free, Nitrile Gloves (4 mil)
34 Extra Large, Powder-Free, Nitrile Gloves (4mil)
35 Disposable Powder Sampling Spatula (300ct)
35 Standard Screening Bin, Selectee (Red)
35 Checkpoint Screening Bowl
36 Standard Screening Bin
36 Standard Screening Bin w/ Hi-Traction
36 X-Ray Marker Kit
37 Large Checkpoint Screening Bin
37 Standard Screening Bin w/ X-Ray Marker
37 Red Stackable Sharps Container - 1 Quart
38 Red Stackable Sharps Container - 2 Gallon
38 Disposable Shoe Covers (50 pair)
38 Screening Bin Rack
39 Distilled Water
39 Distilled Water Dropper
39 Large Cotton Gloves
40 Small Cotton Gloves
40 Isopropyl Alcohol 70%, 16 oz
40 Isopropyl Alcohol 70%, Gallon (4pk)
41 Liquid Peroxide Test Strips 50ct.
41 Membrane Stick
41 Privacy Sheet, 2 Ply Tissue, 40” x 48”
42 Privacy Sheet, 2 Ply Tissue, 40” x 72”
42 Plastic Jug Pump
42 Spray Bottle, 16oz
43 ASTM F 792-88 Stepped Wedge
43 Bottle Label Sticker
43 Dryer Material 500g (Molecular Sieve)
44 Eye Wash Station, 32 oz
44 Eye Wash Station Refill, 32 oz
44 Leak Test Kit
45 Saturated Swabs (25ct)
45 Swab Sampler Disk (10ct)
45 Saturated Alochol Wipes
46 Alcohol Pads (50ct)
46 PTFE Tubing (1/8” ID)
46 Silastic Tubing (1/8” ID)

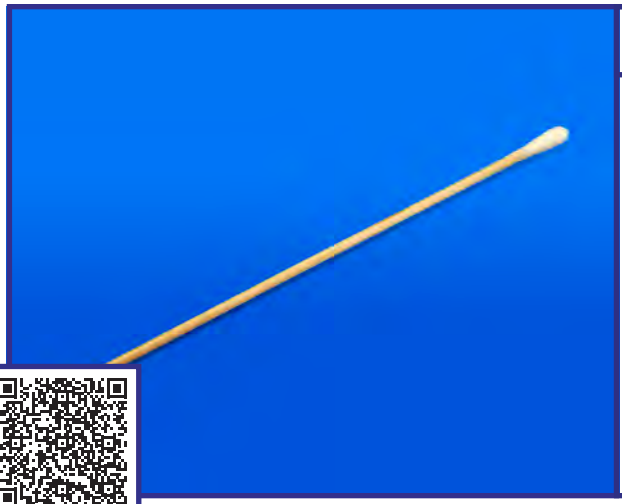


Cotton Swabs (100ct)

SKU: BCS1020

Compatible with: *Checkpoint and Cleaning*

Approval: *DHS Accepted*

Excellent for a range of cleaning purposes. Recommended to be used with Isopropyl Alcohol (70% or greater).

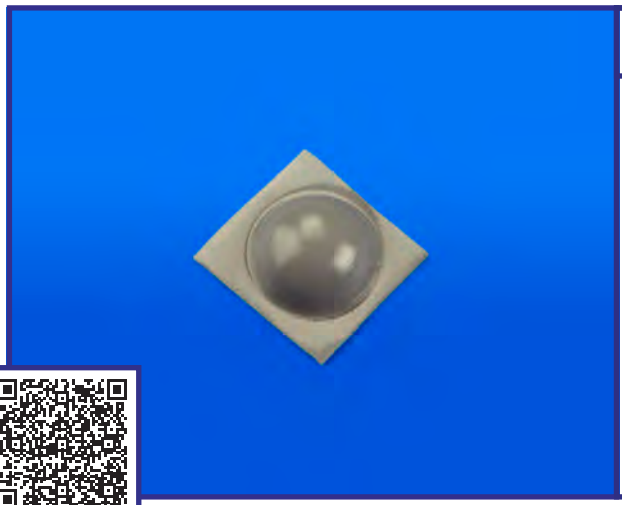


Bumper Feet

SKU: BF1702

Compatible with: *Itemiser® 3/DX/4/5X*

Approval: *DHS*

Bumper feet may become worn or detached and require replacement. Bumper feet are made of self-adhering polyurethane material. The instrument uses eight feet in total, four on the bottom and four on the back for setting it down in an upright position.

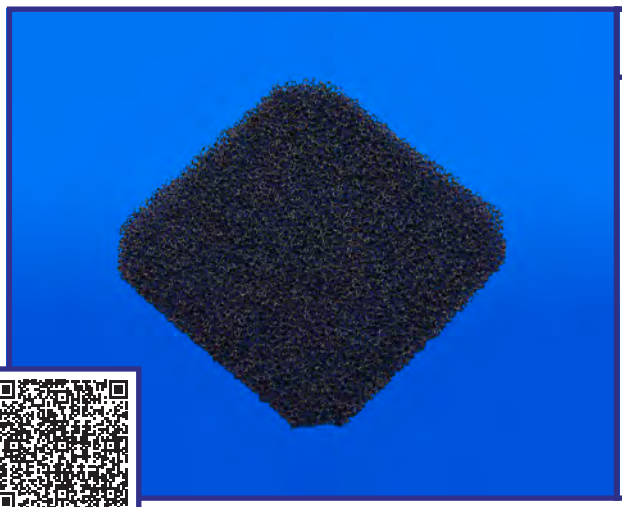

Fan Filter Replacement, 5pk

SKU: BFF1015

Compatible with: *QS-B220™*

Approval: *DHS Accepted*

The fan filter is typically located at the rear of the instrument and is accessible by unsnapping the fan guard. This component filters the cooling air that enters the instrument. Visible dust on the filter is an indication it should be changed immediately.



Sieve Canister X-Ring (#019)

SKU: BOR0180

Compatible with: *QS-B220™*

Approval: *DHS Accepted*

O-rings can occasionally become visually contaminated, damaged or worn and will need to be replaced.




Sieve Canister X-Ring (#012)

SKU: BOR0181

Compatible with: *QS-B220™*

Approval: *DHS Accepted*

O-rings can occasionally become visually contaminated, damaged or worn and will need to be replaced.

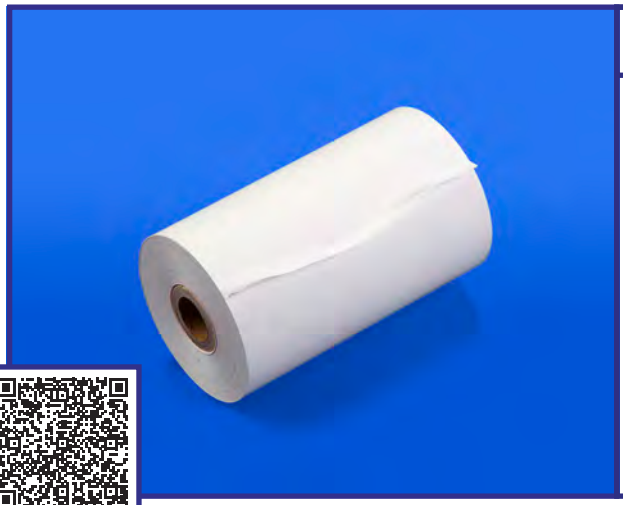

Thermal Paper Roll, 112 mm

SKU: BPP1010

Compatible with: *QS-B220™*

Approval: *DHS Accepted*

The Thermal Printer Paper Rolls are individually packaged in sealed plastic wrappers for freshness.




Verification Sample A - Negative

SKU: BSA1030

Compatible with: *QS-B220™*

Approval: *DHS*

The Verification Sample, A-Negative is used to verify that the ETD instrument is properly calibrated. This product is produced under strict laboratory controls. The Verification Sample, A-Negative is packaged in contaminant-free containers and sealed for maximum freshness and longevity. Please store in a cool, dry place, away from direct sunlight. This product should be stored at room temperature. Clean cotton gloves (GL7500) are required when sampling to prevent contaminants interfering with the performance of the instrument.

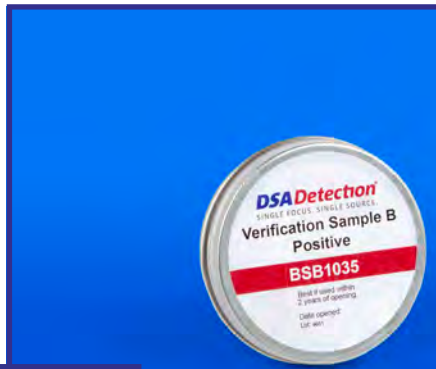


Verification Sample, B - Positive

SKU: BSB1035

Compatible with: *QS-B220™*

Approval: *DHS*

The Verification Sample, B-Positive is used to verify that the ETD instrument is properly calibrated. This product is produced under strict laboratory controls. The Verification Sample, B-Positive is packaged in contaminant-free containers and sealed for maximum freshness and longevity. Please store in a cool, dry place, away from direct sunlight. This product should be stored at room temperature. Clean cotton gloves (GL7500) are required when sampling to prevent contaminants interfering with the performance of the instrument.

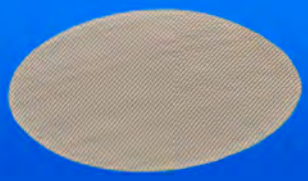

Filter Screen, Sample Pathway

SKU: BSC0001

Compatible with: *QS-B220™*

The filter screen allows target vapors to pass through into the detection system, while blocking out contaminants. During normal use, the filter screen is replaced yearly. In more contaminated environments, the filter screen is replaced as needed.



Filter Screen, Sample Pathway (5ct)

SKU: BSC0002

Compatible with: *QS-B220™*

The filter screen allows target vapors to pass through into the detection system, while blocking out contaminants. During normal use, the filter screen is replaced yearly. In more contaminated environments, the filter screen is replaced as needed.



Orifice Filter Replacement Tool

SKU: BSC1307

Compatible with: *QS-B220™*

Approval: *DHS Accepted*

This tool is used to remove/change the 5-micron filter when doing regular maintenance and changing the four sieve canisters on a QS-B220 instrument.



Sieve Canister (4-pack) with Filter

SKU: BSC1329

Compatible with: *QS-B220™*

Approval: *DHS*

Four canisters and one exterior 5-micron filter are included. The Molecular Sieve Canisters are critical in maintaining proper performance of the QS-B220 instrument and must be replaced periodically. Manufactured in the USA, the QS-B220 Molecular Sieve Canisters have been extensively tested by the DHS Transportation Security Laboratory to ensure they meet or exceed performance standards. Please refer to the instrument manual for installation instructions.



Sieve Canister (12-pack) with Filters

SKU: BSC1340

Compatible with: *QS-B220™*

Approval: *DHS*

Twelve canisters and three exterior 5-micron filter are included. The Molecular Sieve Canisters are critical in maintaining proper performance of the QS-B220 instrument and must be replaced periodically. Manufactured in the USA, the QS-B220 Molecular Sieve Canisters have been extensively tested by the DHS Transportation Security Laboratory to ensure they meet or exceed performance standards. Please refer to the instrument manual for installation instructions.



Alcohol Wipes, 1.7x3.5 (100ct)

SKU: BSW1025

Compatible with: *Checkpoint and Cleaning*

Approval: *DHS Accepted*

Pre-saturated with ultra-pure isopropyl alcohol, these well-constructed wipes resist tears. Excellent for general cleaning of instrument surfaces, they work equally well cleaning harder-to-reach areas.



Calibration Traps, Dual (25ct)

SKU: CT1272P

Compatible with: *QS-B220™, QS-H150E™*

Approval: *DHS*

Calibration Traps are required for proper operation of the instrument. Calibration Traps are produced under strict laboratory controls and are engineered using the highest quality Teflon®-coated (PTFE) fiberglass material available. Calibration Traps meet the exact standards required for precise calibration of your instrument. Traps are packaged in contaminant-free recyclable trays and sealed for maximum freshness and longevity.



B220 Checkpoint Sample Traps (100ct)

SKU: ST1267

Compatible with: *QS-B220™*

Approval: *DHS Checkpoint / Checked Bag Screening*

These advanced sample traps are specifically designed for use in a security checkpoint to collect more particles of interest from various surfaces for analysis. Sample traps are produced under strict laboratory controls and packaged in contaminant-free, recyclable trays. Please store in a cool, dry place, away from direct sunlight. Clean cotton (GL7500, GL7501) or Nitrile gloves (CNG2091, CNG2092, CNG2093, CNG2094) are required when handling sample traps to prevent contaminants from interfering with the performance of the instrument.



B220 Checkpoint Sample Traps (300ct)

SKU: ST1268

Compatible with: *QS-B220™*

Approval: *DHS Checkpoint / Checked Bag Screening*

These advanced sample traps are specifically designed for use in a security checkpoint to collect more particles of interest from various surfaces for analysis. Sample traps are produced under strict laboratory controls and packaged in contaminant-free, recyclable trays. Please store in a cool, dry place, away from direct sunlight. Clean cotton (GL7500, GL7501) or Nitrile gloves (CNG2091, CNG2092, CNG2093, CNG2094) are required when handling sample traps to prevent contaminants from interfering with the performance of the instrument.



Cargo Sample Traps (100ct)

SKU: ST1269P

Compatible with: *QS-B220™, QS-H150E™*

Approval: *DHS Cargo Screening*

DSA is the original manufacturer and the only approved supplier of the QS-B220 sample trap for cargo screening. Sample traps are designed to harvest particles for analysis by the instrument. Sample traps are produced under strict laboratory controls, and packaged in contaminant free recyclable trays. Sample traps should be stored at room temperature away from direct heat. Clean cotton gloves (GL7500, GL7501) are required when handling sample traps to prevent contaminants interfering with the performance of the instrument.



Cargo Sample Traps (300ct)

SKU: ST1270

Compatible with: *QS-B220™, QS-H150E™*

Approval: *DHS Cargo Screening*

DSA is the original manufacturer and the only approved supplier of the QS-B220 sample trap for cargo screening. Sample traps are designed to harvest particles for analysis by the instrument. Sample traps are produced under strict laboratory controls, and packaged in contaminant free recyclable trays. Sample traps should be stored at room temperature away from direct heat. Clean cotton gloves (GL7500, GL7501) are required when handling sample traps to prevent contaminants interfering with the performance of the instrument.



Dual Mode Verification Trap (25ct)

SKU: VT1272

Compatible with: *QS-B220™, QS-H150E™*

Approval: *DHS*

Verification is required to verify that the instrument is properly calibrated. These single-use dual mode verification traps eliminate the need for verification A and verification B canisters, resulting in significant cost savings annually. Dual mode verification traps are produced under strict laboratory controls and are engineered using the highest quality Teflon®-coated (PTFE) fiberglass material available. Traps are packaged in contaminant-free recyclable trays and sealed for maximum freshness and longevity. Clean nitrile gloves are required when handling traps.



Dual Mode Verification Trap (100ct)

SKU: VT1273

Compatible with: *QS-B220™, QS-H150E™*

Approval: *DHS*

Verification is required to verify that the instrument is properly calibrated. These single-use dual mode verification traps eliminate the need for verification A and verification B canisters, resulting in significant cost savings annually. Dual mode verification traps are produced under strict laboratory controls and are engineered using the highest quality Teflon®-coated (PTFE) fiberglass material available. Traps are packaged in contaminant-free recyclable trays and sealed for maximum freshness and longevity. Clean nitrile gloves are required when handling traps.




QS-H150E Sieve Canister

SKU: BSC1210

Compatible with: *QS-H150E™*

The Molecular Sieve Canisters are critical in maintaining proper performance of the QS-H150E instrument and must be replaced periodically. Please refer to the instrument manual for installation instructions.

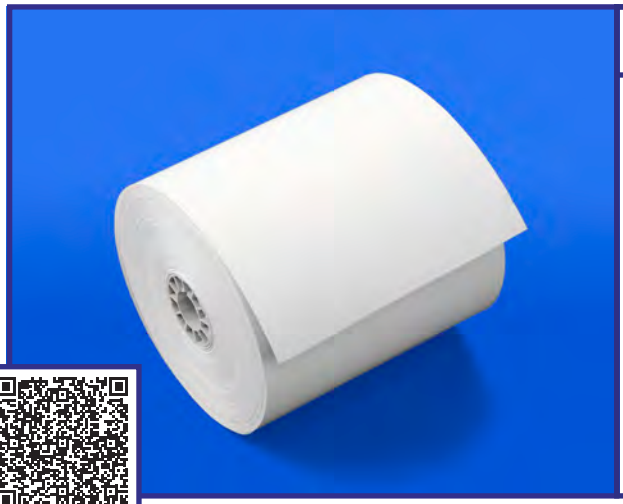

Thermal Printer Paper (80mm)

SKU: DPP4145

Compatible with: *IONSCAN™ 500DT*

Approval: *DHS Accepted*

The thermal printer paper rolls are specifically designed for the IONSCAN™ 500DT & 600DT and matches the manufacturer's OEM part number - 6824145.




Thermal Printer Paper (pkg of 5)

SKU: DPP4146

Compatible with: *IONSCAN™ 500DT*

Approval: *DHS Accepted*

The thermal printer paper rolls are specifically designed for the IONSCAN™ 500DT & 600DT and matches the manufacturer's OEM part number - 6824145.

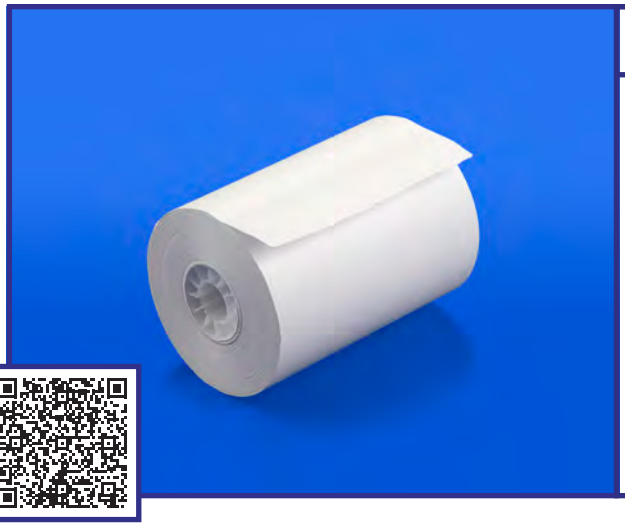

Printer Paper

SKU: DPP8047

Compatible with: *IONSCAN™ 500DT*

Approval: *DHS Accepted*

Impact printer paper is specifically designed for the IONSCAN™ 500DT and matches the manufacturer's specifications precisely for printer part number - 1818777.



Printer Ribbon

SKU: DPR4728

Compatible with: *IONSCAN™ 500DT*

Approval: *DHS Accepted*

Star Micronics printer cartridge, specified for use on the IONSCAN™ 500DT ETD internal printer (part number - 1818777), matches the ETD manufacturer's specifications precisely.



500DT Hand Swab (100ct)

SKU: DSW1205P

Compatible with: *IONSCAN™ 500DT*

Approval: *DHS|STAC*

Hand swabs are designed to sample particles for analysis by an explosive trace detector (ETD). Swabs are packaged in contaminant free recyclable trays and sealed for maximum freshness and longevity. Store in a cool, dry place, away from direct sunlight. Clean cotton gloves (GL7500) are required when handling. Product is also available in quantity 200 (DSW1210P).



500DT Hand Swabs (200ct)

SKU: DSW1210P

Compatible with: *IONSCAN™ 500DT*

Approval: *DHS|STAC*

Hand swabs are designed to sample particles for analysis by an explosive trace detector (ETD). Swabs are packaged in contaminant free recyclable trays and sealed for maximum freshness and longevity. Store in a cool, dry place, away from direct sunlight. Clean cotton gloves (GL7500) are required when handling. Product is also available in quantity 100 (DSW1205P).



500DT Sample Swabs (200ct)

SKU: DSW8055P

Compatible with: *IONSCAN™ 500DT*

Approval: *DHS|STAC*

Our DSA-approved Sample Swabs are designed to sample particles from various surfaces for analysis by the instrument. DSA's Sample swabs are produced under strict laboratory controls and manufactured using the highest quality Nomex® available. Sample Swabs are packaged in contaminant free recyclable trays and sealed for maximum freshness and longevity. Clean cotton gloves (GL7500) are required when handling Sample Swabs. Product is also available in quantity 400 (DSW8066P).



500DT Sample Swabs (400ct)

SKU: DSW8066P

Compatible with: *IONSCAN™ 500DT*

Approval: *DHS|STAC*

Our DSA-approved Sample Swabs are designed to sample particles from various surfaces for analysis by the instrument. DSA's Sample swabs are produced under strict laboratory controls and manufactured using the highest quality Nomex® available. Sample Swabs are packaged in contaminant free recyclable trays and sealed for maximum freshness and longevity. Clean cotton gloves (GL7500) are required when handling Sample Swabs. Product is also available in quantity 200 (DSW8055P).




Sampling Wand Velcro Hook (10ct)

SKU: DVH3347

Compatible with: *IONSCAN™ 500DT*

Approval: *DHS Accepted*

Located at the end of the sampling wand, the Velcro® pad can wear or become contaminated, and thus requires replacement. The Velcro® has a self-adhesive backing for easy installation.

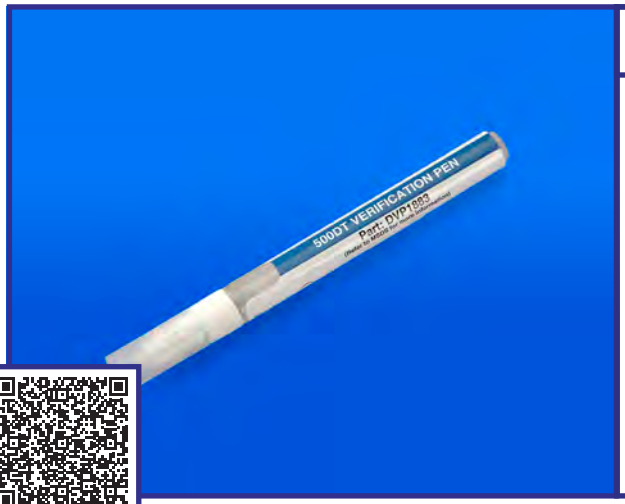

Verification Pen

SKU: DVP1883

Compatible with: *IONSCAN™ 500DT*

Approval: *DHS|STAC*

The Verification Pen is produced under strict laboratory controls, and meets the exact standards required for precise verification of the IONSCAN™ 500DT instrument. The Verification Pen should be stored at room temperature away from direct heat. For extended shelf life, DSA Detection recommends the pen be stored in a refrigerator or freezer. Refer to the label for product instructions. Suitable for cargo use only.




Clearing Dropper

SKU: DWD1004

Compatible with: *IONSCAN™ 500DT*

Approval: *DHS Accepted*

The Clearing Dropper for the 500DT accelerates clear down time after an alarm. This product is produced under strict laboratory quality controls and dispenses a precise amount of clearing solution.

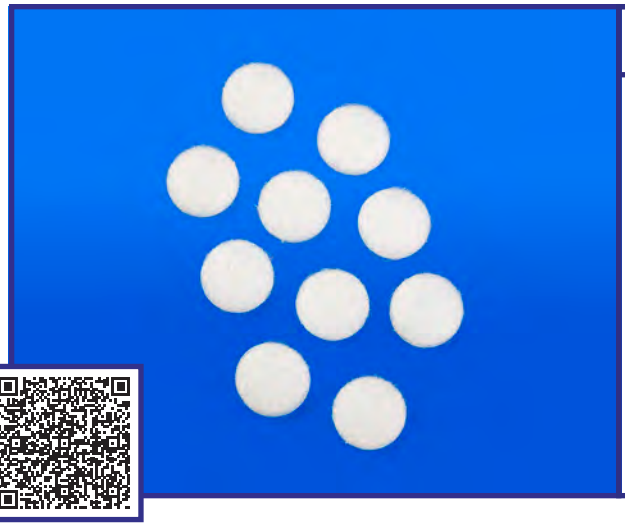

Sampling Wand Velcro Shaper (10ct)

SKU: DWS8944

Compatible with: *IONSCAN™ 500DT*

Approval: *DHS Accepted*

The Velcro® pad is located at the end of the wand where the sample swab is placed. It may wear or become contaminated, thus needing to be replaced.




Itemiser® DX Starter Consumable Kit

SKU: CK1269

Compatible with: *Itemiser® DX*

Approval: *DHS*

Our Itemiser® DX Starter Consumable Kit includes (1) N-Mode Dopant Long Life Positive Ion, (1) E-Mode Dopant Negative Ion, (1) Sample Traps (100ct), (1) Calibration Traps (100ct), (1) Verification Traps (100ct), (1) Canned Air, (1) Clearing Spray, (2) Thermal Printer Paper.

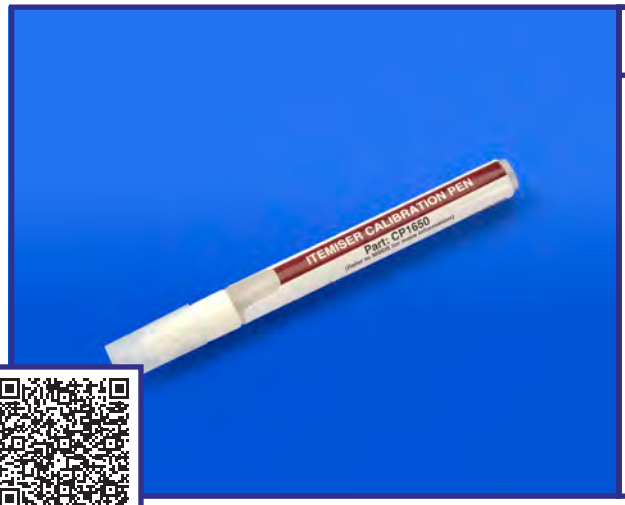

Calibration Pen

SKU: CP1650

Compatible with: *Itemiser® 3/DX/4/5X, VaporTracer2®, MobileTrace®*

The Calibration Pen is produced under strict laboratory controls and meets the exact standards required for precise calibration. The Calibration Pen should be stored at room temperature away from direct heat. For extended shelf life, it is recommended the pen be stored in a refrigerator or freezer. Refer to the label for product instructions.



Clearing Spray

SKU: CS1831

Compatible with: *Itemiser® DX*

Approval: *DHS Accepted*

Our Clearing Spray - 20mL (0.68 fl oz) for the Itemiser® DX accelerates clear down time after an alarm. This product is produced under strict laboratory quality controls and dispenses a precise amount of clearing solution.



Calibration Traps (25ct)

SKU: CT1317P

Compatible with: *Itemiser® 3/DX/4/5X, VaporTracer2®, MobileTrace®*

Approval: *DHS*

Calibration traps are required for proper operation of the instrument. Calibration traps are produced under strict laboratory controls and are engineered using the highest quality Teflon®-coated (PTFE) fiberglass material available. Traps are packaged in contaminant-free recyclable trays and sealed for maximum freshness and longevity. Calibration traps should be stored at room temperature away from direct heat. Clean cotton gloves (GL7500) are required when handling to prevent contaminants from interfering with the performance of the instrument. Calibration traps are single use only.



Calibration Traps (100ct)

SKU: CT1319P

Compatible with: *Itemiser® 3/DX/4/5X, VaporTracer2®, MobileTrace®*

Approval: *DHS*

Calibration traps are required for proper operation of the instrument. Calibration traps are produced under strict laboratory controls and are engineered using the highest quality Teflon®-coated (PTFE) fiberglass material available. Traps are packaged in contaminant-free recyclable trays and sealed for maximum freshness and longevity. Calibration traps should be stored at room temperature away from direct heat. Clean cotton gloves (GL7500) are required when handling to prevent contaminants from interfering with the performance of the instrument. Calibration traps are single use only.




N-Mode Dopant, Long Life Positive Ion

SKU: D1164.

Compatible with: *VaporTracer2®, MobileTrace®*

VaporTracer2® and MobileTrace® Instruments require this product in combination with Negative Ion E-Mode Dopant (D5810) during dual-mode operation. The Long Life, Positive Ion, N-Mode Dopant contains solid ammonia that is released as a gas during the life of the product. Under typical operating conditions, the product will gradually be depleted over an 11-month period as intended. DSA Detection recommends the dopant be refrigerated or frozen to extend its shelf life.

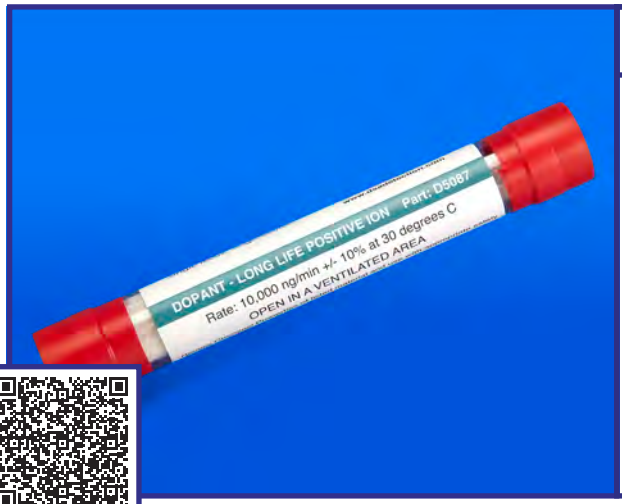

N-Mode Dopant, Long Life Positive Ion

SKU: D5087

Compatible with: *Itemiser® 3/DX/4*

Approval: *DHS*

The Long Life, Positive Ion, N-Mode Dopant contains solid ammonia that is released as a gas during the life of the product. Under typical operating conditions, this product will gradually deplete over an 11-month period. Our product lasts 30% longer than the OEM product. DSA Detection recommends the dopant be stored in a refrigerator or freezer to extend its shelf life.




Sample Filter and Purge Inlet Filter

SKU: FE3224

Compatible with: *Itemiser® 3/DX/4/5X*

Approval: *DHS*

The Sample Filter and Purge Inlet Filter is used to remove contaminants within the air lines.

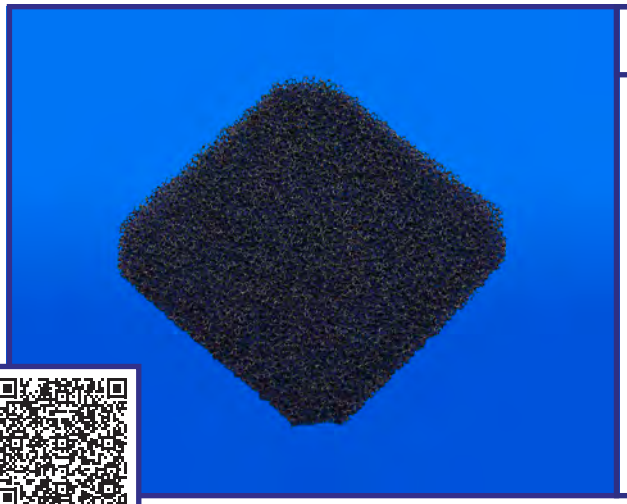


Fan Filter

SKU: FF3222

Compatible with: *Itemiser® 3/DX/4/5X*

Approval: *DHS*

The Fan Filter is typically located at the rear of the instrument and is accessible by unsnapping the fan guard. This component filters the cooling air that enters the instrument. Visible dust on the filter is an indication it should be changed immediately.

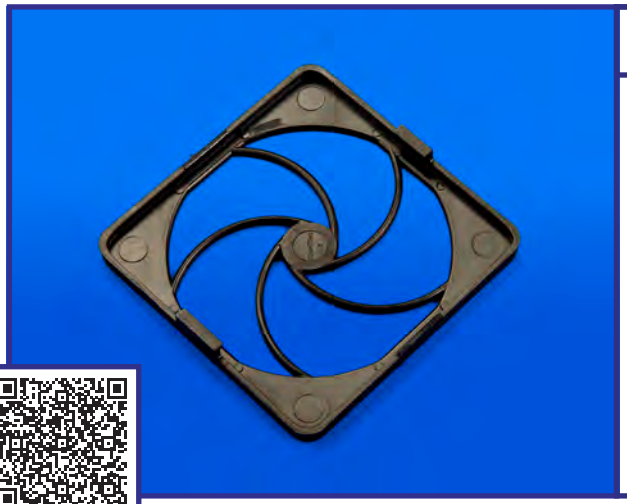

Fan Guard

SKU: FG7125

Compatible with: *Itemiser® 3/DX/4/5X*

Approval: *DHS*

The fan guard is a rigid plastic grill that protects the fan and filter elements from damage and serves as a retainer to hold the filter in place. The guard snaps on and off to service the filter. If you need to replace the fan filter, please reference the instrument manufacturer's replacement instructions.



Fan Filter Kit

SKU: FK3033

Compatible with: *Itemiser® 3/DX/4/5X*

Approval: *DHS*

Kit Contents: Itemiser® DX/3 Fan Guard, Itemiser® DX/3 Fan Filter, Fan Guard Backing.



Fuse, 250V AC 3.15A

SKU: FS2500

Compatible with: *Itemiser® DX/4/5X, VaporTracer2®*

Approval: *DHS*

Direct replacement for OEM P/N EP002500. 3.15A Type T 5x20mm.



Fuse, 15A, 32V 3AG, for DC input

SKU: FS2525

Compatible with: *Itemiser® 3/DX/4/5X*

Approval: *DHS*

Direct replacement for OEM P/N EP002525.




Nozzle Screen Kit

SKU: NK5282

Compatible with: *Itemiser® DX*

Approval: *DHS*

The Nozzle Screen Kit contains (6) screens that allow target vapors to pass through into the detection system. The kit also contains a Nozzle Removal Tool. Generally, the Nozzle Screen is replaced during monthly maintenance; but harsh operating environments may require more frequent changing. At a minimum, the Nozzle Screen should be inspected weekly and cotton gloves (Large GL7500, Small GL7501) should be worn while servicing the instrument. For installation, follow instrument manufacturer's procedures.

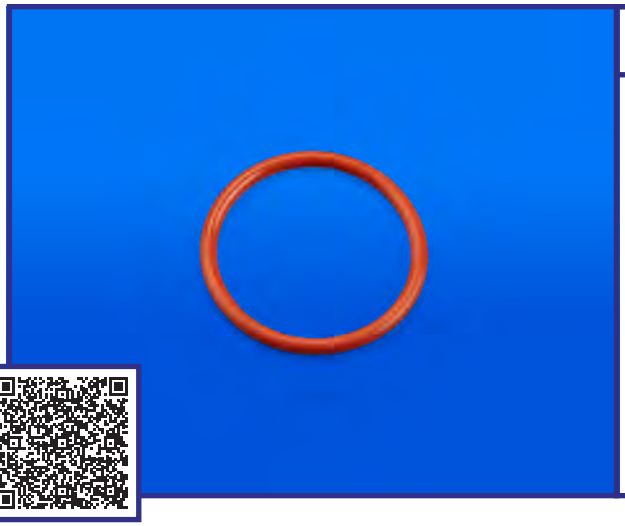


O-Ring Silicone (#019)

SKU: OR1060

Compatible with: *Itemiser® 3/DX/4/5X*

Approval: *DHS*

O-rings can occasionally become visually contaminated, damaged or worn and will need to be replaced.

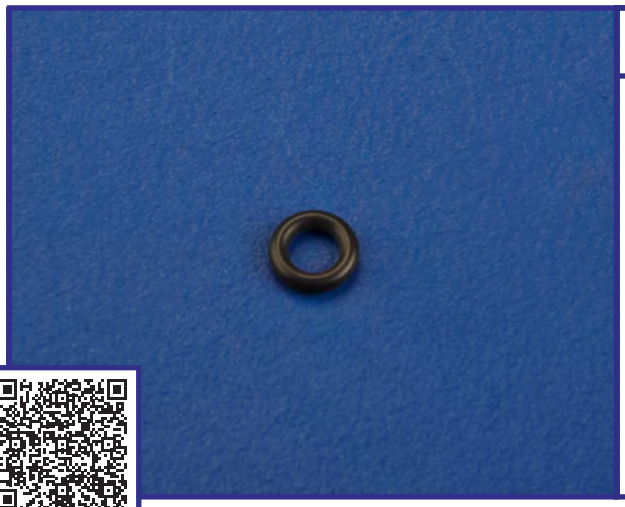


O-Ring Viton (#008)

SKU: OR1108

Compatible with: *Itemiser® DX/3/2*

Approval: *DHS*

O-rings can occasionally become visually contaminated, damaged or worn and will need to be replaced.

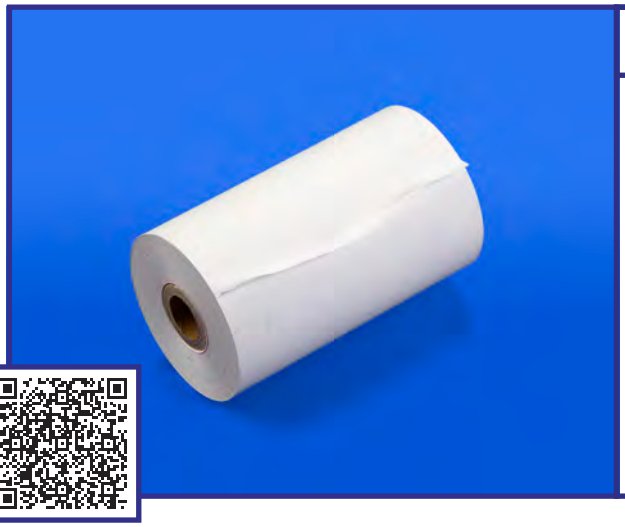

Thermal Printer Paper

SKU: PP5060

Compatible with: *Itemiser® 5X/DX/3/2*

Approval: *DHS*

The thermal printer paper rolls are individually packaged in sealed plastic wrappers for freshness.



Spare Parts Kit

SKU: SK5141

Compatible with: *Itemiser® 3*

This Maintenance Kit contains commonly used parts to keep your instrument in service and avoid downtime. All items are easily replaced in the field. Kit contents include: Fuse 220V AC 3.15A Qty (2), Fuse 15A 32V 3AG For DC Input Qty (1), O-Ring Silicone .8125ID Qty (1), Sample Air Filter Rubber Washer Qty (1), Sintered Filter Qty (1), O-Ring .176ID Qty (2).



Itemiser® 3/DX Spare Parts Kit

SKU: SK5284

Compatible with: *Itemiser® DX*

Approval: *DHS*

This spare parts kit contains commonly used parts to keep your instrument in service and avoid downtime. All the items are easily replaced in the field. Kit contents include (4) Bumper Feet, (1) 15A 32V 3AG DC Input Fuse, (2) 220V AC 3.15A Fuses, (1) O-Ring Silicone .8125ID, *(1) O-Ring Silicone .301ID. *This item not sold separately.



Sample Traps (25ct)

SKU: ST1316P

Compatible with: *Itemiser® 3/DX/4/5X, VaporTracer2®, MobileTrace®*

Approval: *DHS and DfT*

Sample traps are designed to harvest particles from various surfaces for analysis by the instrument. Sample traps are produced under strict laboratory controls and manufactured using the highest quality Teflon®-coated (PTFE) fiberglass material available. Traps are packaged in contaminant free recyclable trays and sealed for maximum freshness and longevity. Sample traps should be stored at room temperature away from direct heat. Clean cotton gloves (GL7500) are required when handling to prevent contaminants from interfering with the performance of the instrument.



Itemiser Sample Traps (100ct)

SKU: ST1318P

Compatible with: *Itemiser® 3/DX/4/5X , VaporTracer2®, MobileTrace®*

Approval: *DHS and DfT*

Sample traps are designed to harvest particles from various surfaces for analysis by the instrument. Sample traps are produced under strict laboratory controls and manufactured using the highest quality Teflon®-coated (PTFE) fiberglass material available. Traps are packaged in contaminant free recyclable trays and sealed for maximum freshness and longevity. Sample traps should be stored at room temperature away from direct heat. Clean cotton gloves (GL7500) are required when handling to prevent contaminants from interfering with the performance of the instrument.




Itemiser Sample Traps (300ct)

SKU: ST1322P

Compatible with: *Itemiser® 3/DX/4/5X, VaporTracer2®, MobileTrace®*

Approval: *DHS and DfT*

Sample traps are designed to harvest particles from various surfaces for analysis by the instrument. Sample traps are produced under strict laboratory controls and manufactured using the highest quality Teflon®-coated (PTFE) fiberglass material available. Traps are packaged in contaminant free recyclable trays and sealed for maximum freshness and longevity. Sample traps should be stored at room temperature away from direct heat. Clean cotton gloves (GL7500) are required when handling to prevent contaminants from interfering with the performance of the instrument.

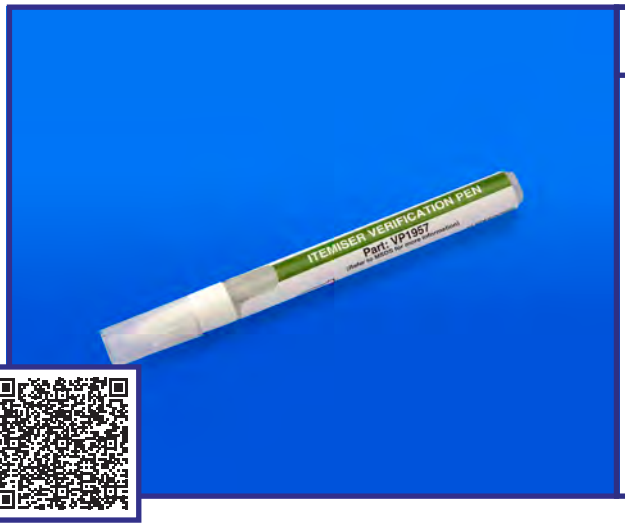

Verification Pen

SKU: VP1957

Compatible with: *Itemiser® 3/DX/4/5X, VaporTracer2®, MobileTrace®*

The Verification Pen is produced under strict laboratory controls and meets the exact standards required for precise verification of the instrument. The Verification Pen should be stored at room temperature away from direct heat. For extended shelf life, DSA Detection recommends the pen be stored in a refrigerator or freezer. Refer to the label for product instructions.



Verification Traps (100ct)

SKU: VT1336P

Compatible with: *Itemiser® 3/DX/4/5X, VaporTracer2®, MobileTrace®*

Approval: *DHS*

Verification traps are required to verify that the instrument is properly calibrated. Verification traps are produced under strict laboratory controls. Traps are packaged in contaminant-free recyclable trays and sealed for maximum freshness and longevity. Verification traps should be stored at room temperature away from direct heat. Clean cotton gloves (GL7500, GL7501) are required when handling verification traps to prevent contaminants from interfering with the performance of the instrument. Verification traps are single use and should not be reused.



Verification Traps (25ct)

SKU: VT1337P

Compatible with: *Itemiser® 3/DX/4/5X, VaporTracer2®, MobileTrace®*

Approval: *DHS*

Verification traps are required to verify that the instrument is properly calibrated. Verification traps are produced under strict laboratory controls. Traps are packaged in contaminant-free recyclable trays and sealed for maximum freshness and longevity. Verification traps should be stored at room temperature away from direct heat. Clean cotton gloves (GL7500, GL7501) are required when handling verification traps to prevent contaminants from interfering with the performance of the instrument. Verification traps are single use and should not be reused.



Check Sample Vial - Military

SKU: SV1172M

Compatible with: *MobileTrace®*

Use the check sample vial to verify the instrument's proper calibration and detection capability. Check sample vials should be stored at room temperature away from direct heat.



Sintered Filter

SKU: SF3001

Compatible with: *Itemiser® 3/2*

Approval: *DHS*

The sintered filter removes contaminants from the instrument's air supply. Inspect monthly and replace when visibly dirty. For installation, follow instrument manufacturer's procedures.




Condenser Tube

SKU: SCT5030

Compatible with: *IONSCAN™ 400B*

Approval: *DHS*

Condenser tubes are designed to remove contaminants within air lines. They are manufactured to perform equal to or better than the OEM product. For installation, follow instrument manufacturer's procedures.

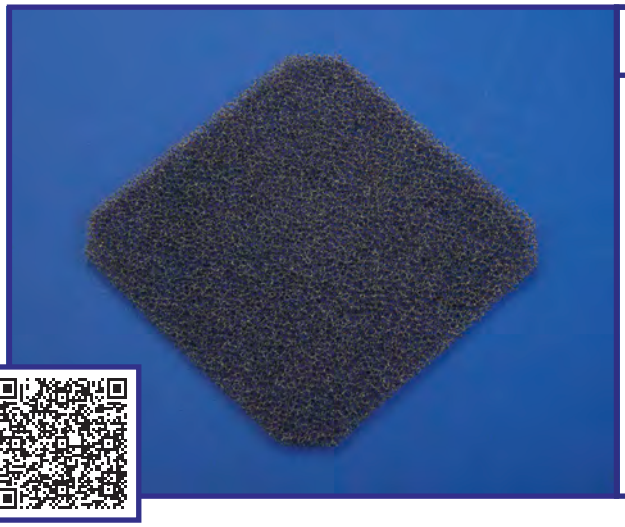


Foam Filter

SKU: SFF1654

Compatible with: *IONSCAN™ 400B/500DT*

Approval: *DHS*

The fan filter filters cooling air as it enters the instrument. To access, unsnap the fan guard on the back panel of the instrument. The frequency with which the filter requires changing depends on the operating environment; however visible dust on the filter indicates it should be changed immediately.

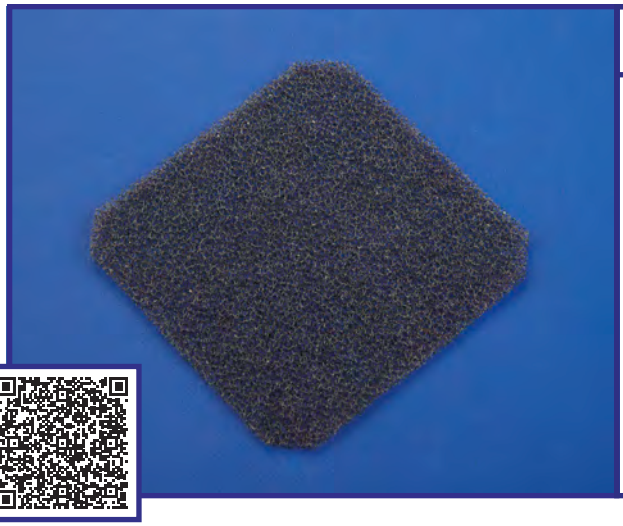


Behind Bottle Foam Filter

SKU: SFF3222

Compatible with: *IONSCAN™ 400B*

Approval: *DHS*

The Foam Filter filters the cooling air as it enters the rear of the instrument. The frequency with which the filter requires changing depends on the operating environment; however visible dust on the filter indicates it should be changed immediately.

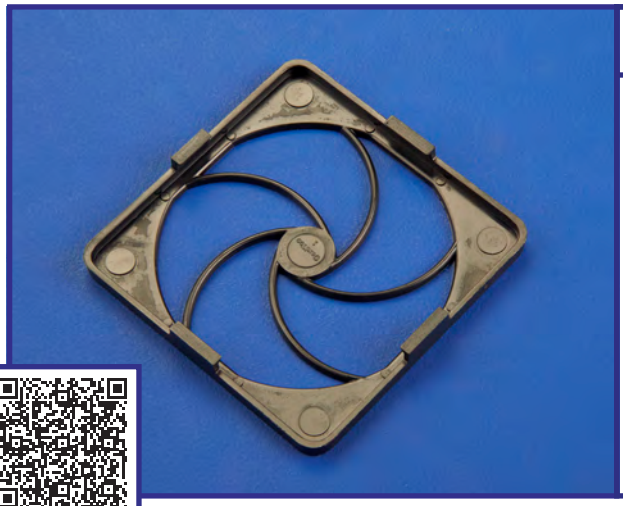


Fan Guard, 4-Prong

SKU: SFG0280

Compatible with: *IONSCAN™ 400B*

Approval: *DHS*

The fan guard is a rigid plastic grill that protects the fan and filter elements from damage and serves as a retainer to hold the filter in place. The guard snaps on and off to service the filter.

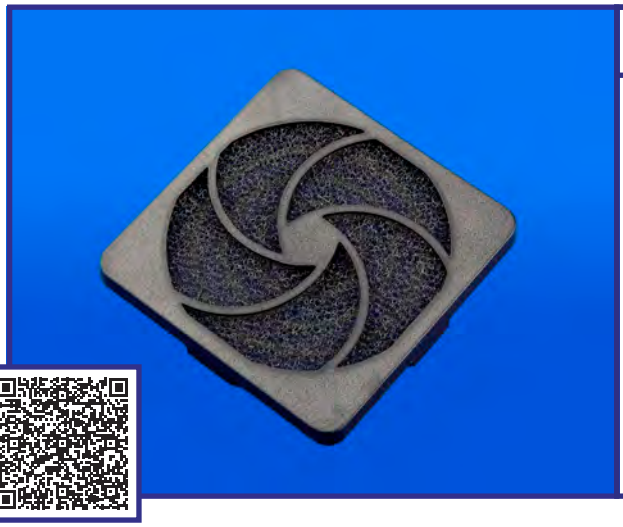

Behind Bottle Cover and Filter

SKU: SFK0279

Compatible with: *IONSCAN™ 400B*

Approval: *DHS*

Frequency of changing the filter is dependent on the atmosphere in which the instrument is operating, however when dust becomes visible on the filter, this is an indication it should be changed immediately.



Filter Kit

SKU: SFK9230

Compatible with: *IONSCAN™ 400B/500DT*

Approval: *DHS*

The fan filter kit includes front and rear plastic fan guards, and a fan filter. The purpose is to filter the cooling air that enters the rear of the instrument. Frequency of changing the filter is dependent on the atmosphere in which the instrument is operating, however when dust becomes visible on the filter, this is an indication it should be changed immediately.



O-ring, Viton (#009)

SKU: SOR3730

Compatible with: *IONSCAN™ 400B*

Approval: *DHS Accepted*

O-rings can occasionally become visually contaminated, damaged or worn and will need to be replaced.




O-ring, Viton (#012)

SKU: SOR5330

Compatible with: *IONSCAN™ 400B*

Approval: *DHS Accepted*

O-rings can occasionally become visually contaminated, damaged or worn and will need to be replaced.

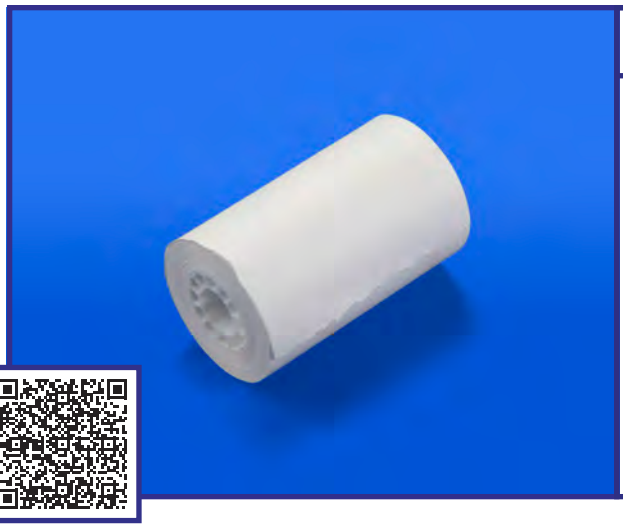


400B Printer Paper, Intl

SKU: SPP0601

Compatible with: *IONSCAN™ 400B*

Packaged in sealed wrappers for freshness, this printer paper is specified by the printer manufacturer. Highly recommended to use only original printer manufacturer paper to avoid damage.

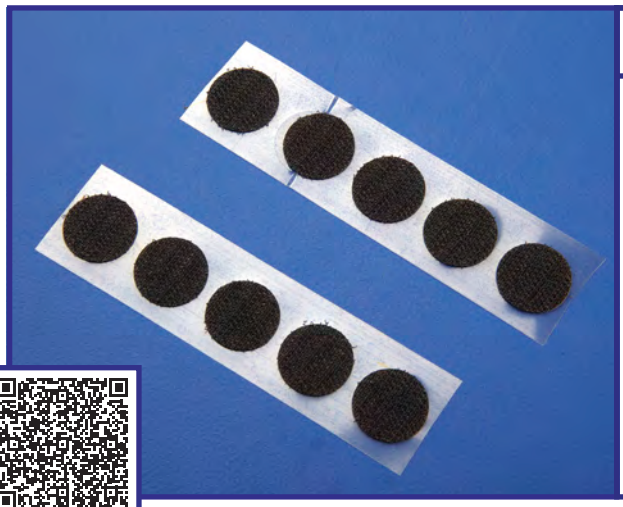

Swab Sampler Velcro Hook (10ct)

SKU: SVH5038

Compatible with: *IONSCAN™ 400B*

Approval: *DHS|STAC*

Located at the end of the sampling wand, the Velcro® pad can wear or become contaminated, and thus requires replacement. The Velcro® has a self-adhesive backing for easy installation.




CW/TIC Vapor Verific

SKU: ASV2919

Compatible with: *SABRE™ 4000/5000*

Approval: *DHS*

For use in CW/TIC vapor mode to verify the instrument is properly calibrated. For use, follow instrument manufacturers procedures. The vapor verific vial should be stored at room temperature away from direct heat.

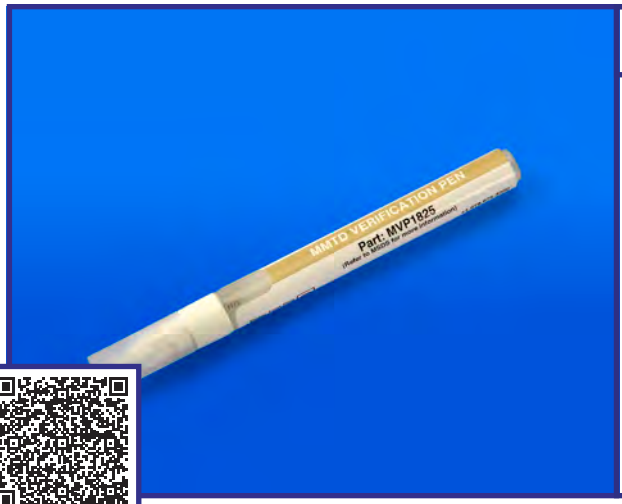

Verification Pen

SKU: MVP1825

Compatible with: *SABRE™ 4000/5000*

The Verification Pen is produced under strict laboratory controls, and meets the exact standards required for precise verification of the SABRE 4000/5000 and MMTD instrument. The Verification Pen should be stored at room temperature away from direct heat. For extended shelf life, DSA Detection recommends the pen be stored in a refrigerator or freezer. Refer to the label for product instructions.




Membrane Kit

SKU: MK5007

Compatible with: *Itemiser® 3/2, VaporTracer2®, MobileTrace®*

Approval: *DHS*

The membrane kit contains five semi-permeable elastomeric membranes that allow target vapors to pass through into the detection system. Generally, the membrane is replaced during monthly maintenance; but harsh operating environments may require more frequent changing of the membrane. At a minimum, the membrane should be inspected weekly and cotton gloves (GL7500) should be worn while servicing the membrane. For installation, follow instrument manufacturer's procedures.

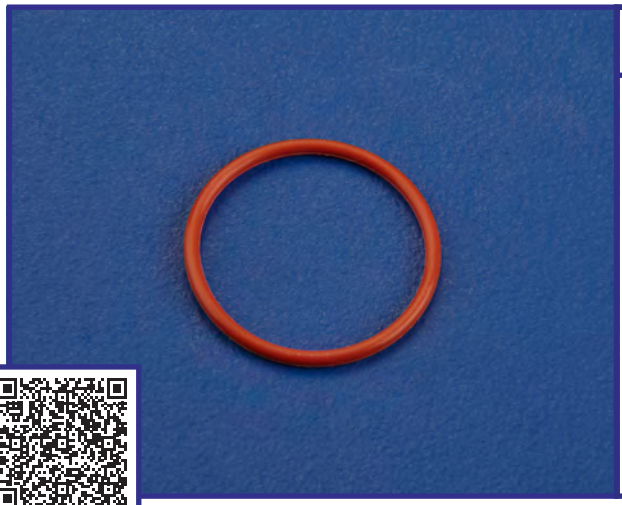

O-Ring Silicone (#022)

SKU: OR1102

Compatible with: *Itemiser® 2, VaporTracer2®, MobileTrace®*

Approval: *DHS*

O-rings can occasionally become visually contaminated, damaged or worn and will need to be replaced.



Canned Air

SKU: CA7503

Compatible with: *Checkpoint and Cleaning*

Approval: *DHS*

The "DusteR" canned air has an air stream of .2 microns to clean critical components and areas of trace instruments. Hold can upright—never inverted, tilted, or shaken—and apply in short bursts several inches from the target area to avoid damage to fragile components. This is OEM recommended, not the flammable and less-pure canned air product available from office supply stores. Please note: Due to supply chain issues, canned air pricing is subject to change at any moment.



Standard Bin Cart

SKU: CBC4400

Compatible with: *All*

Approval: *DHS Accepted*

Key Features of our 20 1/2" x 32 1/2" Standard Bin Cart include non-marking casters, 2 pre-drilled permanent bins and hardware, a 250 lb load capacity, and a 50 bin capacity. Some assembly required. Adjustable wrench recommended. For use with DSA's Standard Bin (CSB3349). Also compatible with this product are DSA bins with X-ray markers (CSBX3349) and traction (CSB3351).



Safety Enclosure Cleaning Cloth

SKU: CC4003

Compatible with: *Checkpoint and Cleaning*

Approval: *DHS Accepted*

The Safety Enclosure Cleaning Cloth is used with the liquid scanner to clean the sensitive glass area. Also used with VT or any other instrument that has a glass portion or an LCD screen.



ETD Mobile Workstation (powered)

SKU: CMW4000

Compatible with: *All*

Approval: *DHS Accepted*

Key Features of our ETD Mobile Powered Workstation include adjustable push handle, locking wheels, 3"" tall locking drawer, three sided shelf lip 1.5"" high, binder holder, Top Shelf: 22"" wide x 24"" deep. Battery Specifications include power pack including two (2) fully enclosed 100 Amp hr AGM, deep cycle industrial batteries charged with standard 120V outlet, warranted for 6 months, expected life-cycle is two years with proper use, integrated 15 amp power strip with 6 outlets, eight foot power cord.



ETD Mobile Powered Workstation LiFePO4

SKU: CMW6000

Compatible with: *All*

Approval: *DHS Accepted*

Key Features of our ETD Mobile Powered Workstation include adjustable push handle, locking wheels, 3"" tall locking drawer, three sided shelf lip 1.5"" high, binder holder, Top Shelf: 22"" wide x 24"" deep. Battery Specifications include 1 Lithium Iron Phosphate Battery, with a charge time of 7.5 hours. This battery has an 8-10 year lifetime rated for 3,000 power cycles.



Replacement Batteries for Mobile Workstation (2pk)

SKU: CMWB206

Compatible with: *All*

Approval: *DHS Accepted*

Battery Kit includes: two fully enclosed 100 Amp hr AGM Deep cycle industrial batteries charged with standard 120V outlet. The battery is warranted for 6 months and has an expected life cycle is two years with proper use.



Inverter/Charger 1000w, Mobile Workstation

SKU: CMWB235

Compatible with: *All*

1000W Inverter/Charger for use with the Mobile Workstation.



LiFePO4 Battery

SKU: CMWB279

Compatible with: *All*

Approval: *DHS Accepted*

Upgrading to the NEW power source (lithium iron phosphate) has many proven benefits over the previous battery model (sealed lead acid): Only 1 battery required vs. 2, Battery lasts 8-10 years vs. 1-2, Battery weighs 32 lbs vs. 140, Battery lasts 3,000 charge/discharge cycles vs. 300. Other benefits include: Improved worker safety, much easier to move on cart, weighs 100 lbs less than the previous battery model, new smart battery with Bluetooth user interface.



Small, Powder-Free, Nitrile Gloves (4mil)

SKU: CNG2091

Compatible with: *Checkpoint and Cleaning*

Wearing disposable gloves while operating or maintaining instruments is extremely important to avoid contamination from the natural oils, dirt, and lotions typically found on hands that can adversely affect the instrument's ability to analyze. Also available in Medium (CNG2092), Large (CNG2093), and Extra Large (CNG2094).



Medium, Powder-Free, Nitrile Gloves (4mil)

SKU: CNG2092

Compatible with: *Checkpoint and Cleaning*

Wearing disposable gloves while operating or maintaining instruments is extremely important to avoid contamination from the natural oils, dirt, and lotions typically found on hands that can adversely affect the instrument's ability to analyze. Also available in Small (CNG2091), Large (CNG2093), and Extra Large (CNG2094).



Large, Powder-Free, Nitrile Gloves (4 mil)

SKU: CNG2093

Compatible with: *Checkpoint and Cleaning*

Wearing disposable gloves while operating or maintaining instruments is extremely important to avoid contamination from the natural oils, dirt, and lotions typically found on hands that can adversely affect the instrument's ability to analyze. Also available in Small (CNG2091), Medium (CNG2092), and Extra Large (CNG2094).



Extra Large, Powder-Free, Nitrile Gloves (4mil)

SKU: CNG2094

Compatible with: *Checkpoint and Cleaning*

Wearing disposable gloves while operating or maintaining instruments is extremely important to avoid contamination from the natural oils, dirt, and lotions typically found on hands that can adversely affect the instrument's ability to analyze. Also available in Small (CNG2091), Medium (CNG2092), and Large (CNG2093).



Disposable Powder Sampling Spatula (300ct)

SKU: CPS0001

Compatible with: *Checkpoint and Cleaning*

These Disposable Powder Sampling Spatulas are designed to remove a powder sample for analysis without contaminating the source.



Standard Screening Bin, Selectee (Red)

SKU: CSB1529

Compatible with: *All*

Approval: *DHS Accepted*

Our red screening bin is used primarily as a "selectee identifier" for passengers going through a checkpoint. Dimensions for this bin are 21.5"L x 15.75"W x 5"H. Not compatible with our Bin Cart (CBC4400). The selectee screening bin can be combined with the X-ray marker kit (CSB3500). We also offer bins with X-ray markers (CSBX3349) and traction (CSB3351).



Checkpoint Screening Bowl

SKU: CSB1801

Compatible with: *All*

The first bowl designed with checkpoint security in mind. Designed and manufactured in New England, this bowl has a low profile and a grippy overmolded base to ensure it doesn't tip over and will make it through heavy X-ray curtains. This bowl is compatible with all X-ray and CT systems and will not effect automatic detection.



Standard Screening Bin

SKU: CSB3349

Compatible with: *All*

Approval: *DHS Accepted*

Our Standard Screening Bin (Dimensions: 20"L x 15"W x 5"H) is the same one used across all airports by the TSA. We always have stock ready to ship. The screening bin is the most durable available and conveniently stacks on our Screening Bin Cart (CBC4400). We also offer bins with X-ray markers (CSBX3349) and traction (CSB3351).



Standard Screening Bin w/ Hi-Traction

SKU: CSB3351

Compatible with: *All*

Approval: *DHS Accepted*

DSA's hi-traction bin (20"L x 15"W x 5"H) is able to move lighter items through the lead curtains of the X-ray machine. Traction pads are permanent, durable, non-abrasive and do not affect bin stackability. DSA testing determined that a hi-traction screening bin could carry about 60-70% less weight through the lead curtains of an X-ray machine, when compared to a standard screening bin without traction. Still compatible with the same portable screening bin cart currently used in 465 +/- airports: CBC4400.



X-Ray Marker Kit

SKU: CSB3500

Compatible with: *All*

Approval: *DHS*

Now, screeners can easily identify bins for secondary screening by their individual numbers, visible by sight and while positioned in an X-ray system tunnel. X-ray markers are permanent, durable, and do not affect bin stackability. Only compatible with DSA screening bins CSB3349, CSB1529, and CSB3351.



Large Checkpoint Screening Bin

SKU: CSB4001

Compatible with: *All*

Approval: *DHS*

The Large Security Checkpoint Screening Bin was designed to hold the largest size dimensions permitted by airlines for carry-on luggage. Compatible with Advanced Technology (AT-2) carry-on baggage screening systems. When bins are stacked 30 high, they are stable without tilting or falling over when moved from point to point. This bin DOES NOT have RFID functionality. Buy American Act compliant, this product is 100% designed and manufactured in New England.



Standard Screening Bin w/ X-Ray Marker

SKU: CSBX3349

Compatible with: *All*

Approval: *DHS*

Introducing the first and only DHS/TSA/TSL/TSIF-approved numbered screening bin (20"L x 15"W x 5"H) that is X-ray correct. Now, screeners can easily identify bins for secondary screening by their individual numbers, visible by sight and while positioned in an X-ray system tunnel. X-ray markers are permanent, durable, and do not affect bin stackability! Compatible with screening bin cart used in 465 +/- airports: CBC4400. We also offer x-ray marker kits (CSB3500). Only compatible with DSA screening bins CSB3349 and CSB3351.



Red Stackable Sharps Container - 1 Quart

SKU: CSC0001

Compatible with: *All*

With a locking lid, the SHARPS-tainer™ provides a safe and convenient way to dispose of and transport needles, lancets, syringes, and other sharp objects. An optional steel bracket for wall mounting is also available by request.



Red Stackable Sharps Container - 2 Gallon

SKU: CSC0002

Compatible with: *All*

With a locking lid, the SHARPS-tainer™ provides a safe and convenient way to dispose of and transport needles, lancets, syringes, and other sharp objects. An optional steel bracket for wall mounting is also available by request.




Disposable Shoe Covers (50 pair)

SKU: CSC4600

Compatible with: *All*

Approval: *DHS Accepted*

One size fits all. Latex and lint free polypropylene shoe covers. These shoe covers are clean-room compliant and have an elastic opening that provides a snug fit around the ankle.

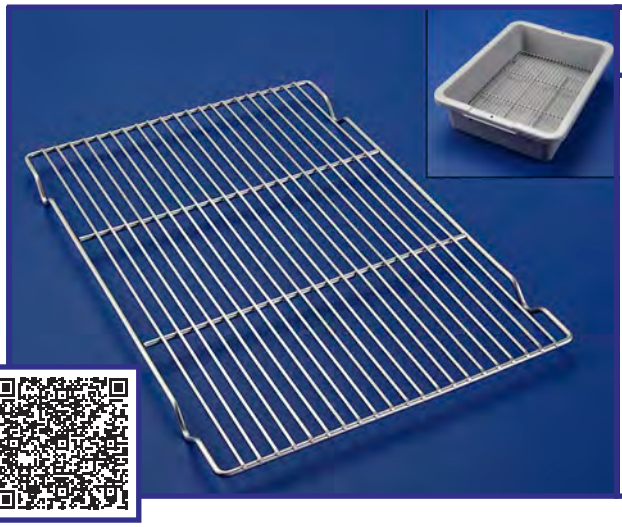

Screening Bin Rack

SKU: CSR5491

Compatible with: *All*

Approval: *DHS Accepted*

The chrome-plated metal rack fits neatly inside the bottom of our gray screening bin and is used when screening objects such as funeral urns. We also offer bins with X-ray markers (CSBX3349) and traction (CSB3351).



Distilled Water

SKU: DW0003

Compatible with: *All*

Approval: *DHS Accepted*

Distilled water is excellent for a range of uses at checkpoint.



Distilled Water Dropper

SKU: DWD1005

Compatible with: *All*

Approval: *DHS Accepted*

The Distilled Water Dropper is for use with test strips. This product is produced under strict laboratory quality controls.



Large Cotton Gloves

SKU: GL7500

Compatible with: *Checkpoint and Cleaning*

Approval: *DHS*

Wearing cotton gloves while operating or maintaining the instrument is extremely important to avoid contamination from the natural oils, dirt, and lotions typically found on hands that can adversely affect the instrument's ability to analyze. Made of pure cotton, these gloves absorb perspiration and allow the hands to "breathe" for greater operator comfort while protecting the sample. Frequent changing to fresh gloves is recommended and required after an alarm.



Small Cotton Gloves

SKU: GL7501

Compatible with: *Checkpoint and Cleaning*

Approval: *DHS*

Wearing cotton gloves while operating or maintaining the instrument is extremely important to avoid contamination from the natural oils, dirt, and lotions typically found on hands that can adversely affect the instrument's ability to analyze. Made of pure cotton, these gloves absorb perspiration and allow the hands to "breathe" for greater operator comfort while protecting the sample. Frequent changing to fresh gloves is recommended and required after an alarm.



Isopropyl Alcohol 70%, 16 oz

SKU: IA0002

Compatible with: *Checkpoint and Cleaning*

Approval: *DHS Accepted*

70% Isopropyl Alcohol. Excellent for a range of cleaning purposes. Use with Cotton Swabs (BCS1020) and Spray Bottle (SB1686).



Isopropyl Alcohol 70%, Gallon (4pk)

SKU: IA2128

Compatible with: *Checkpoint and Cleaning*

Approval: *DHS Accepted*

70% Isopropyl Alcohol. Excellent for a range of cleaning purposes. Perfect for cleaning with cotton swabs and for use with DSA's spray bottle. Sanitizes 99.9% of germs. Sold by the case, 4 gallons per case. Orders over qty. 5 will ship on a pallet. HAZMAT fees and standard delivery without special instructions are included in the price for TSA customers. There is currently no limit on order quantities. Air Shipment (Overnight, 2nd Day, OCONUS) possible. Contact us for a quote.




Liquid Peroxide Test Strips 50ct.

SKU: LTS0001

Compatible with: *Checkpoint and Cleaning*

These TSA test strips are used to detect oxidizing agents, in particular peroxides. The level of sensitivity is ~1 ppm (part per million) in solutions. The strips may also react with other oxidizers (such as chlorine, bromine, and some acids). The development of a blue color indicates the presence of an oxidizer.

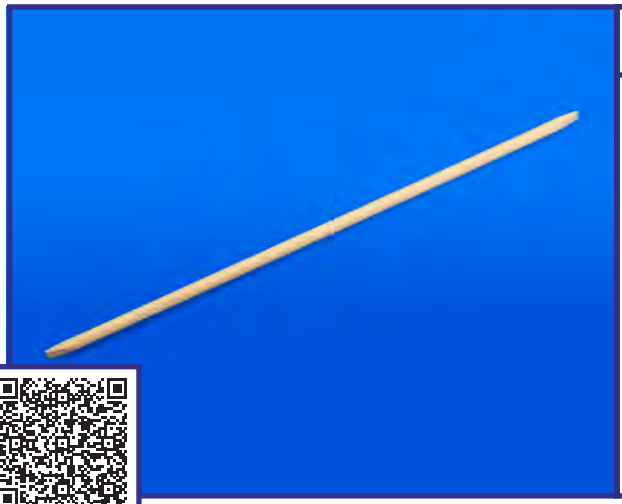

Membrane Stick

SKU: MS5226

Compatible with: *Itemiser® 3/2, VaporTracer2®, MobileTrace®*

Approval: *DHS*

Use the soft membrane stick to remove the membrane or sintered filter while performing maintenance to avoid scratching the detector nozzle during membrane removal.



Privacy Sheet, 2 Ply Tissue, 40” x 48”

SKU: PS0001

Compatible with: *All*

Approval: *DHS Accepted*

Use to protect passenger privacy during searches at security checkpoints.



Privacy Sheet, 2 Ply Tissue, 40” x 72”

SKU: PS0002

Compatible with: *All*

Approval: *DHS Accepted*

Use to protect passenger privacy during searches at security checkpoints.



Plastic Jug Pump

SKU: PU0001

Compatible with: *All*

For dispensing liquids. Perfect fit for Isopropyl Alcohol (IA128). Fits 1/2 gal. and 1 gal. F-style jugs, utility jugs and square utility jugs. Spout rotates 360°. FDA compliant. Polypropylene with flexible 11” intake tube.



Spray Bottle, 16oz

SKU: SB1686

Compatible with: *Checkpoint and Cleaning*

Approval: *DHS Accepted*


Perfect for use around the checkpoint for cleaning ETD stainless steel tables and cabinets. The Spray Bottle is refillable with Isopropyl Alcohol (IA0002).



ASTM F 792-88 Stepped Wedge

SKU: TSK9288

The ASTM-F792-88 Step Wedge is made of ASTM No. 1100 Aluminum or equivalent and is10" long, consisting of 10 one-inch steps with five copper wires with plastic insulation, and are 22, 24, 26, 28, and 30 AWG (American Wire Gage) in diameter.The ASTM-F792-88 Step Wedge is used to meet the needs for testing sophisticated X-raysystems and was developed to strictly comply with FAA and TSA requirements.This standard has been superseded by ASTM F792-17e1.

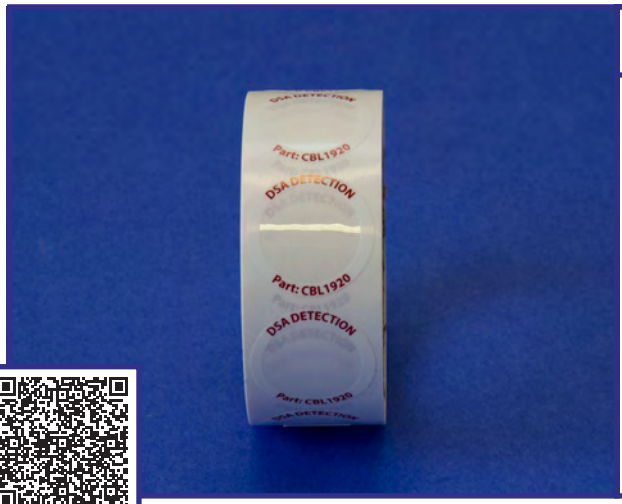

Bottle Label Sticker

SKU: CBL1920

Compatible with: *All*

Approval: *DHS Accepted*

Bottled liquids scanner screening systems differentiate liquid explosives from common, benign liquids. BLS units use a variety of technologies including lasers, infrared, and electromagnetic resonance. Current units screen clear and tinted glass and plastic bottles. DSA Detection's sticker label allows the laser to pass through a non-clear or frosted glass. Once the sticker is attached to the surface of the frosted container, the operator aligns it with the laser, and the liquid is evaluated.



Dryer Material 500g (Molecular Sieve)

SKU: DM5019

Compatible with: *Itemiser® 2, VaporTracer2®, MobileTrace®*

Approval: *DHS*

The molecular sieve removes moisture and contaminants from the instruments air lines. For installation, follow instrument manufacturer's procedures.



Eye Wash Station, 32 oz

SKU: EW0001

Compatible with: *All*

Approval: *DHS Accepted*

Eye Wash stations provide immediate relief after accidents. Packaged for high visibility, each wall unit is designed for easy access for emergency flushing and decontamination of the eyes, face and body. Wall stations mount easily with provided fasteners. Also available are Eye Wash Station Refills (EW0002).



Eye Wash Station Refill, 32 oz

SKU: EW0002

Compatible with: *All*

Approval: *DHS Accepted*

This refill consists of two 32 fl. oz. bottles of sterile isotonic eyewash solution.To be used with the EW0001 Eye Wash Station, 32 oz.



Leak Test Kit

SKU: LT0001

Compatible with: *All*

The radiation leak test kit is required semiannual to comply with regulations. For detailed instructions, refer to the included wipe test kit instructions and the maintenance/troubleshooting section of your user's manual. Kit contents include cotton swabs, decontamination wipes, leak test instructions, and a fully addressed envelope.




Saturated Swabs (25ct)

SKU: SS7502

Compatible with: *Checkpoint and Cleaning*

Approval: *DHS*

Use pre-saturated CHEM SWABS™ for routine cleaning and maintenance of sensitive, hard-to-reach areas, such as the membrane on the detector nozzle, where dust and dirt can reduce instrument sensitivity. Made of urethane foam, these non-abrasive swabs are saturated with alcohol which evaporates quickly and leaves no residue or contamination.

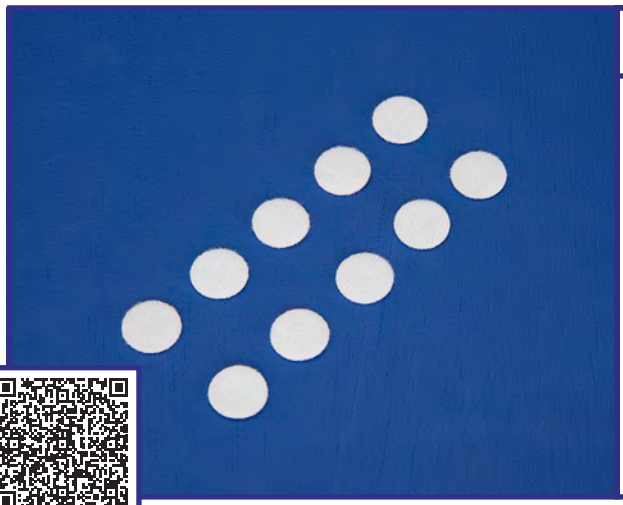

Swab Sampler Disk (10ct)

SKU: SSD5278

Compatible with: *IONSCAN™ 400B*

Approval: *DHS*

The Velcro® pad is located at the end of the wand where the sample swab is placed. It may wear or become contaminated, thus needing to be replaced.



Saturated Alochol Wipes

SKU: SW7501

Approval: *DHS*

Pre-saturated with ultra-pure isopropyl alcohol, these well-constructed wipes resist tears and linting. Excellent for general cleaning of instrument surfaces, they work equally well cleaning hard-to-reach areas.This item may not be shipped by air.




Alcohol Pads (50ct)

SKU: SW7507

Compatible with: *Checkpoint and Cleaning*

Approval: *DHS*

Pre-saturated with ultra-pure isopropyl alcohol, these well-constructed wipes resist tears and linting. Excellent for general cleaning of instrument surfaces, they work equally well cleaning hard-to-reach areas.

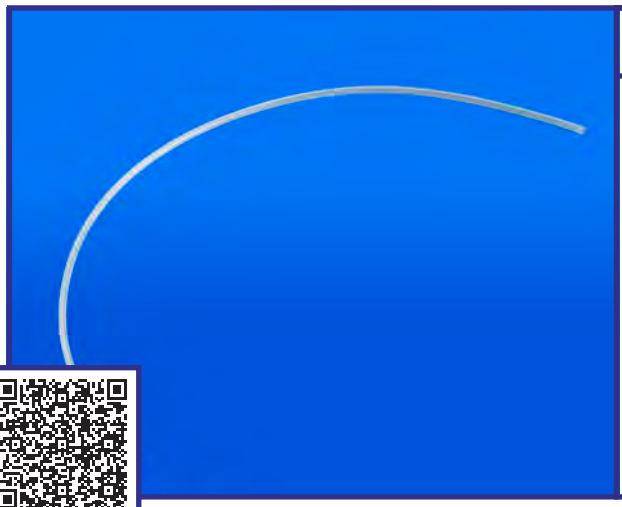


PTFE Tubing (1/8” ID)

SKU: TU8043

Compatible with: *All*

Approval: *DHS*

PTFE tubing can occasionally become visually contaminated, damaged or worn and will need to be replaced. Sold by the foot.

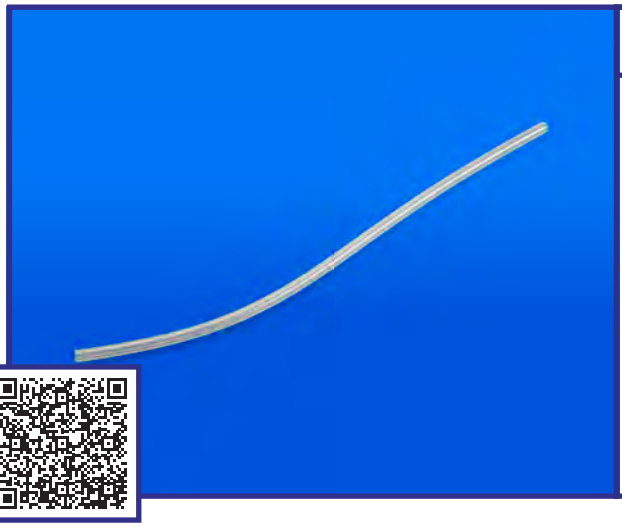

Silastic Tubing (1/8” ID)

SKU: TU8047

Compatible with: *Itemiser® 3/DX/4/5X , VaporTracer2®, MobileTrace®*

Approval: *DHS*

Silastic tubing can occasionally become visually contaminated, damaged or worn and will need to be replaced. Sold by the foot.